


Hexarelin HPLC Test Result

Date: 11/1/2019

一、Test Method:

Column: :C18. 4.6*250mm, 5um
Solvent B :100% Acetonitrile
Solvent A :0.1% Trifluoroacetic in 100% Water
Gradient : B A
0.0min 25% 75%
30.0min 55% 45%
Flow Rate :1.0ml/min
Wavelength :220nm
Temperature :37°C
Concentration :0.5mg/ml
Sample Volume :20ul

二、Auto-Scaled Chromatogram:

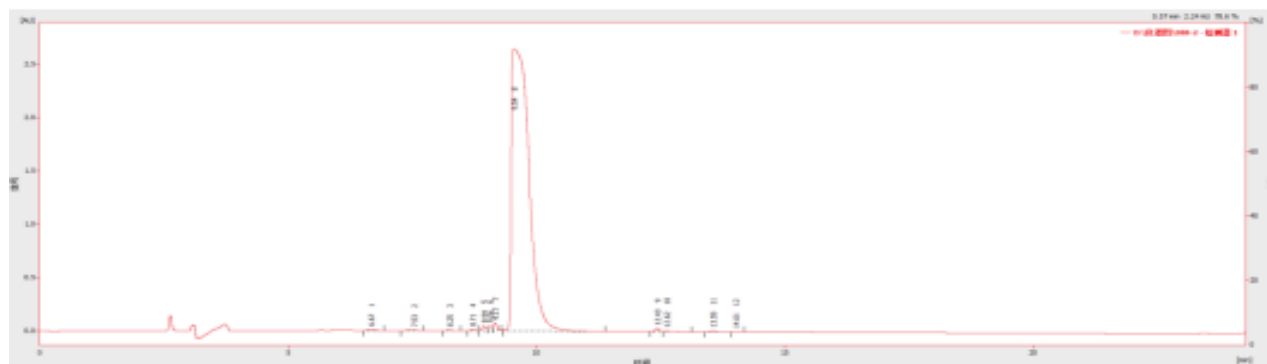

三、Result:

	RT [min]	ST [min]	ET [min]	Area [mAU.s]	Area [%]
1	6.668	6.503	6.932	72.358	0.1
2	7.532	7.264	7.707	35.573	0.1
3	8.248	8.100	8.469	27.183	0.0
4	8.709	8.605	8.820	56.045	0.1
5	8.940	8.838	9.002	223.278	0.3
6	9.057	9.002	9.119	242.922	0.4
7	9.172	9.119	9.290	356.779	0.5
8	9.545	9.301	11.378	64407.825	98.0
9	12.430	12.286	12.542	171.868	0.3
10	12.616	12.542	13.116	50.653	0.1
11	13.554	13.375	13.915	91.004	0.1
12	14.013	13.915	14.173	10.504	0.0
	Total			65745.991	100.0