


Mass Spectrum

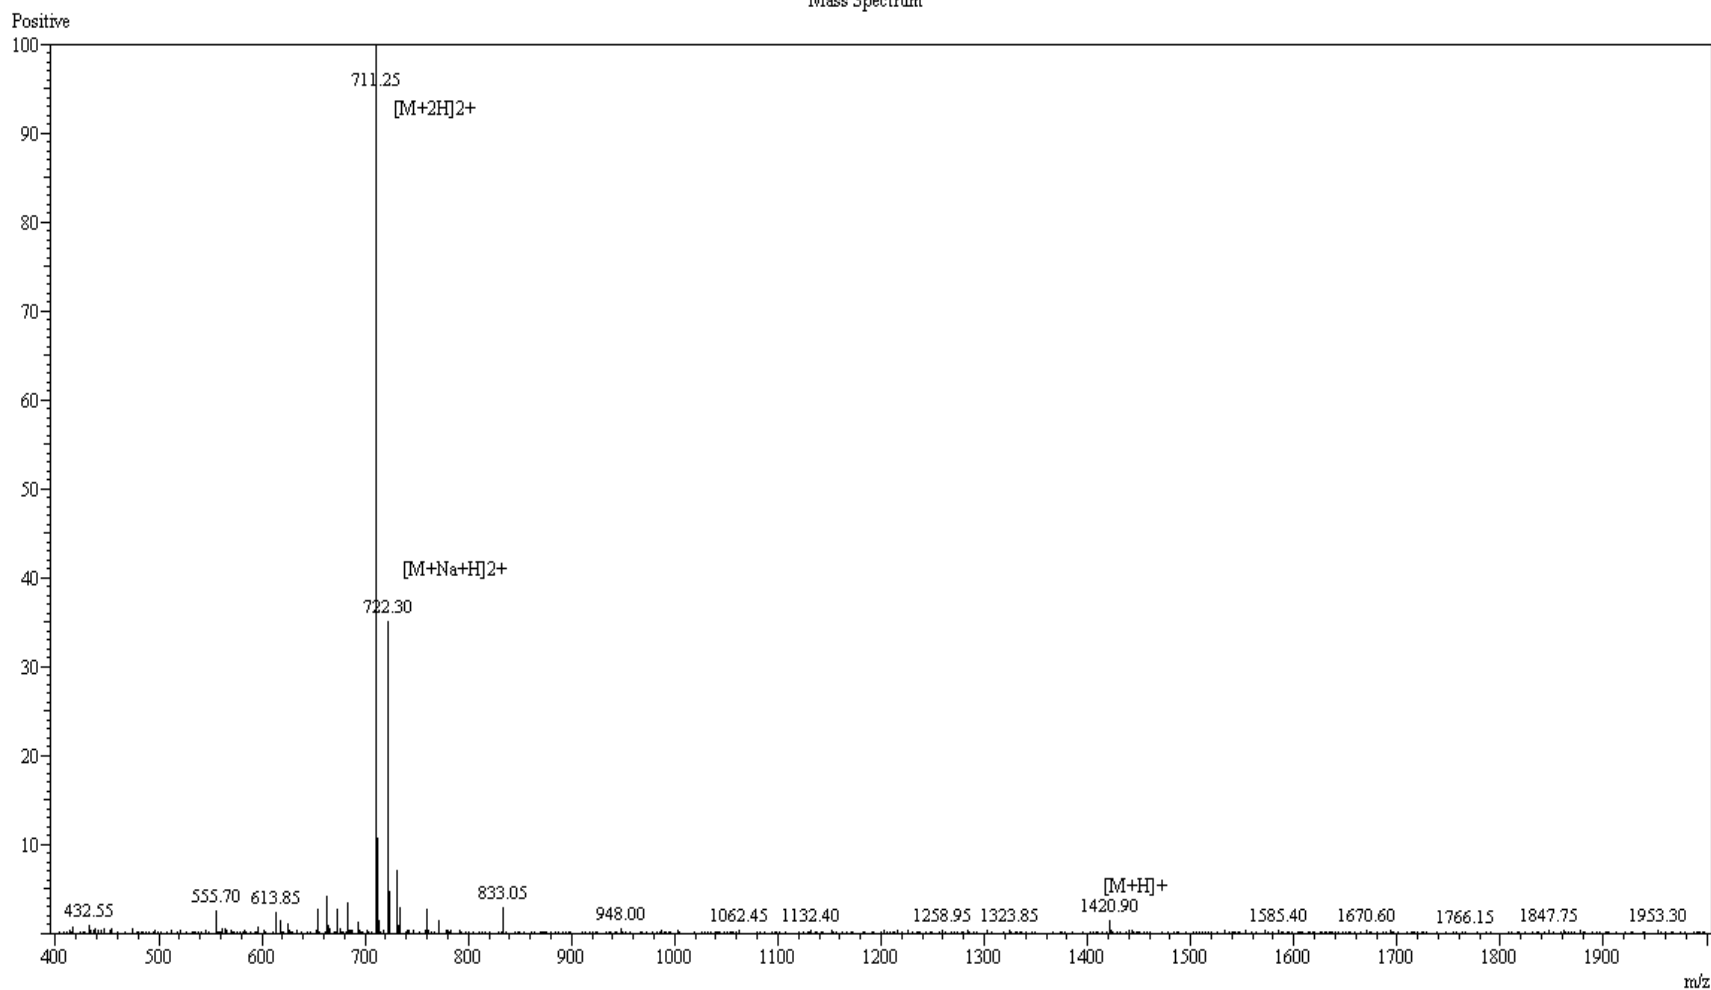

Sample :BPC157
MW : 1419.57
Lot No : P1901028-LR076014

Probe:	ESI	Probe bias:	+4.5kv
Nebulizer Gas Flow:	1.5L/min	Detector:	1.5kv
CDL:	-20.0v	T. Flow:	0.2ml/min
CDL Temp:	250°C	B. conc:	50% H2O/50% ACN
Block Temp:	200°C		