


REPORT

Sequence :

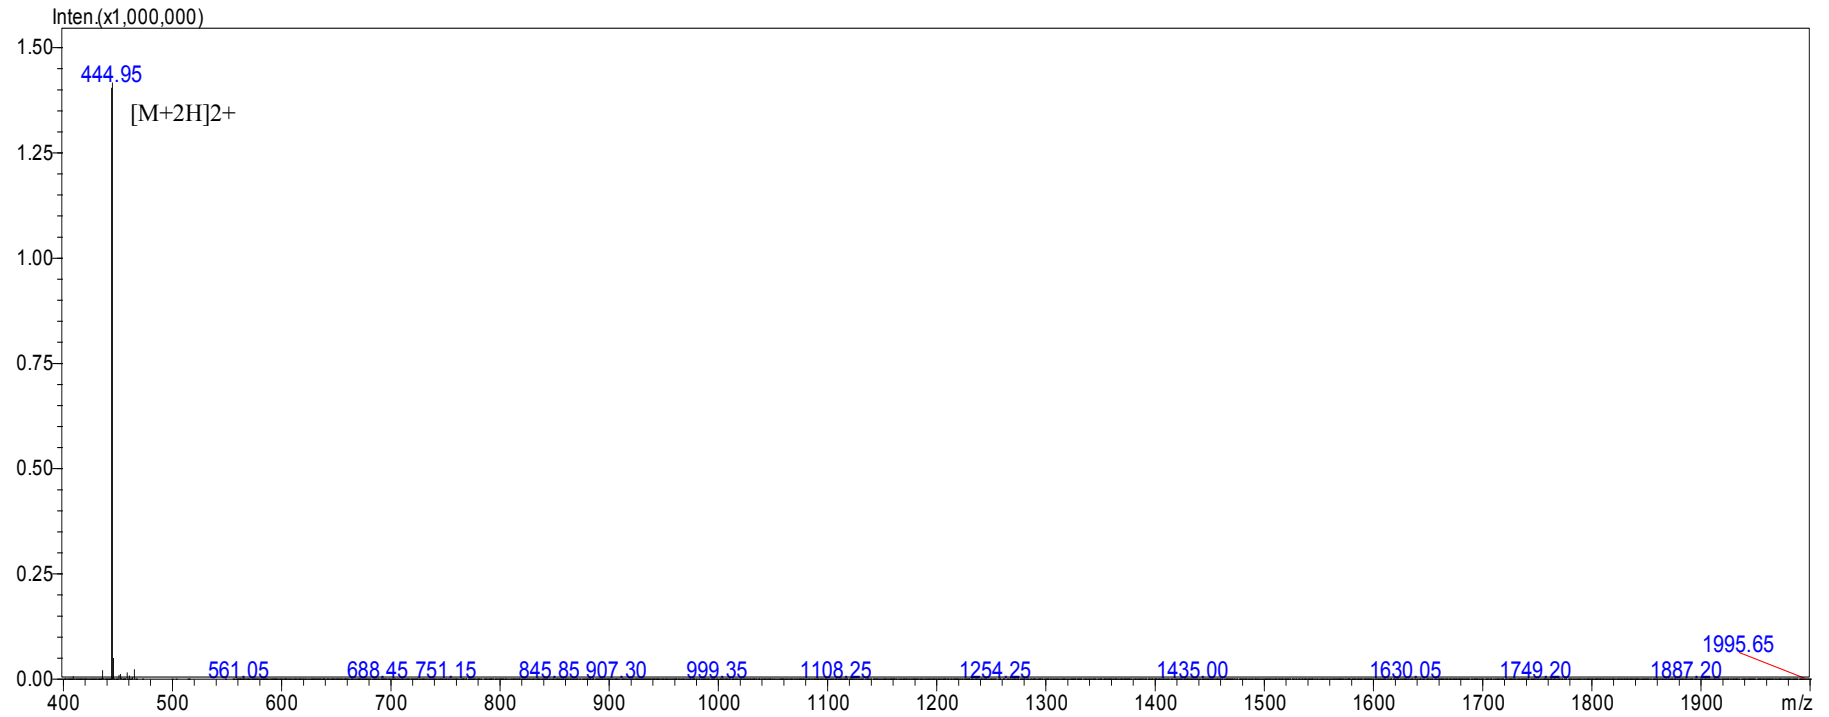

Date and Time: 2019-11-25 12:45:30
Sample : Hexarelin
MW : 887.0
Lot No. : P191111-LR050701

Probe: ESI
Nebulizer Gas Flow: 1.5L/min
CDL: -20.0v
CDL Temp: 250°C
Block Temp: 200°C

Probe bias: +4.5kv
Detector: 1.5kv
T. Flow: 0.2ml/min
B. conc: 50%H2O/50%ACN