


REPORT

Sequence :

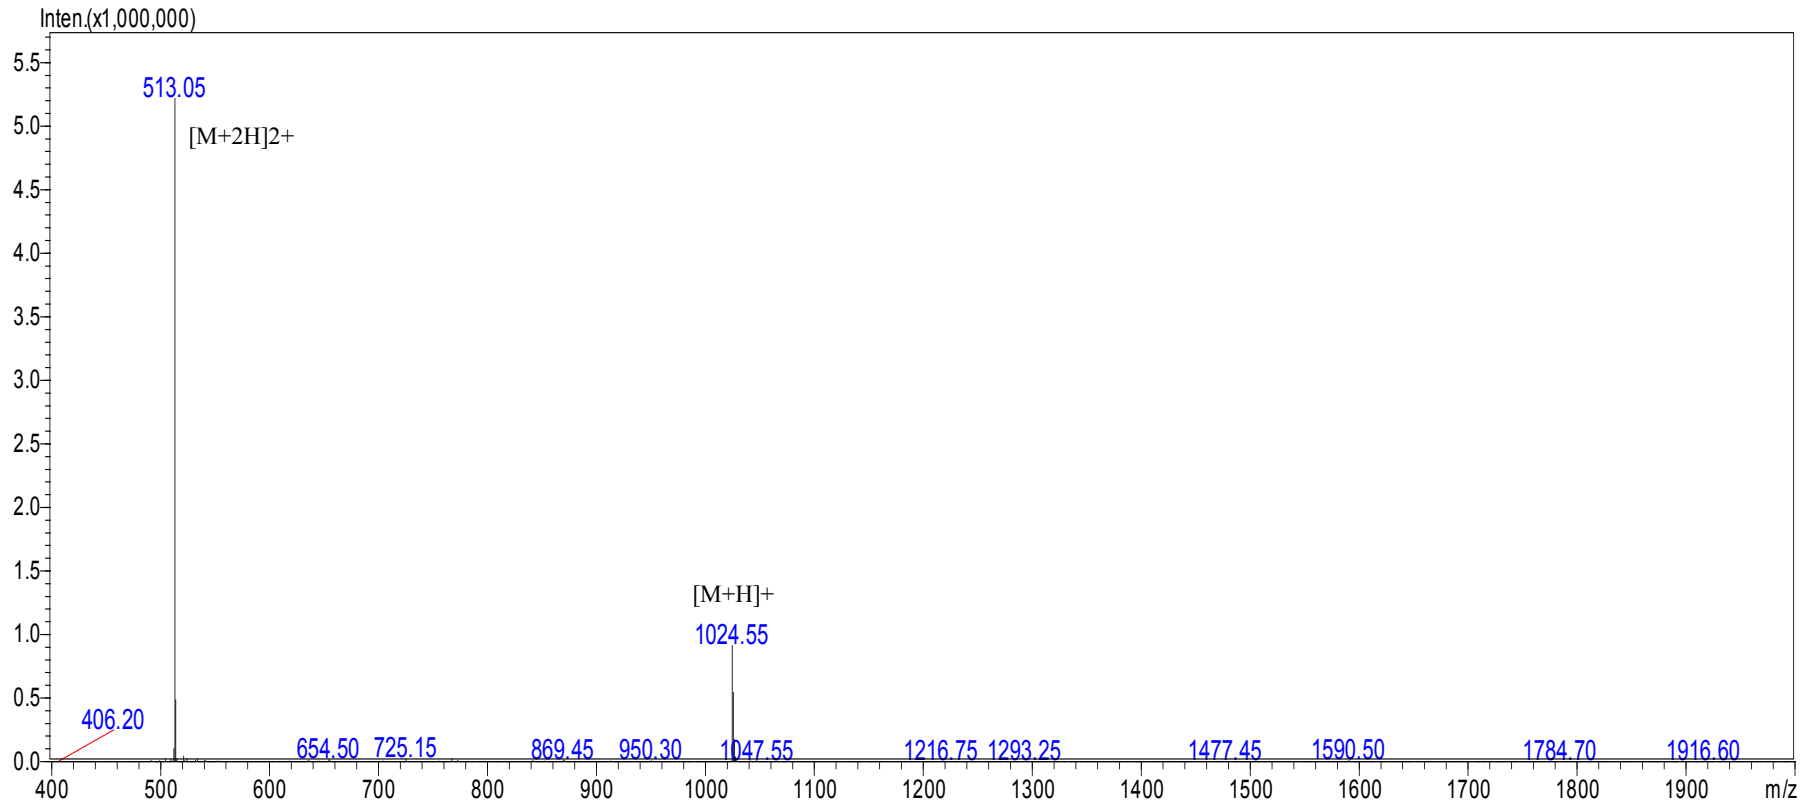

Date and Time: 2019-11-25 13: 30:27

Sample : Melanotan II

MW : 1024.2

Lot No. : P191104-LR052189

Probe: ESI  
Nebulizer Gas Flow: 1.5L/min  
CDL: -20.0v  
CDL Temp: 250°C  
Block Temp: 200°C

Probe bias: +4.5kv  
Detector: 1.5kv  
T. Flow: 0.2ml/min  
B. conc: 50%H2O/50%ACN