


REPORT

Sequence : :

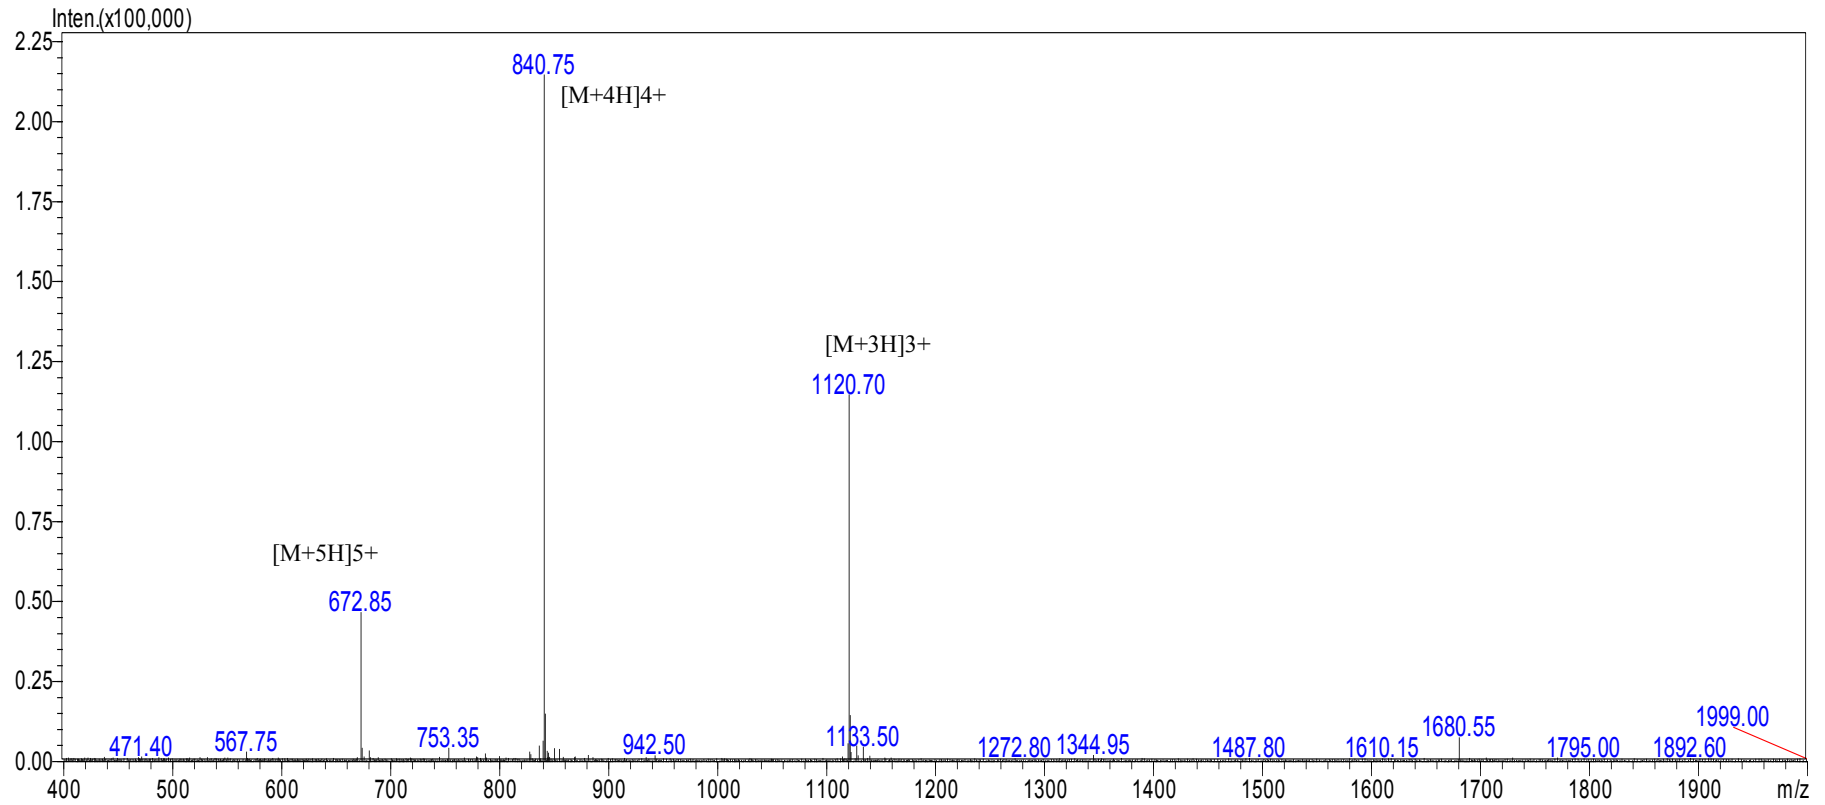

Date and Time: 2019-11-25 12:50:23
Sample : Sermorelin
MW : 3358.03
Lot No. : P191105-LR061712

Probe: ESI
Nebulizer Gas Flow: 1.5L/min
CDL: -20.0v
CDL Temp: 250°C
Block Temp: 200°C

Probe bias: +4.5kv
Detector: 1.5kv
T. Flow: 0.2ml/min
B. conc: 50%H2O/50%ACN