


REPORT

Sequence : :

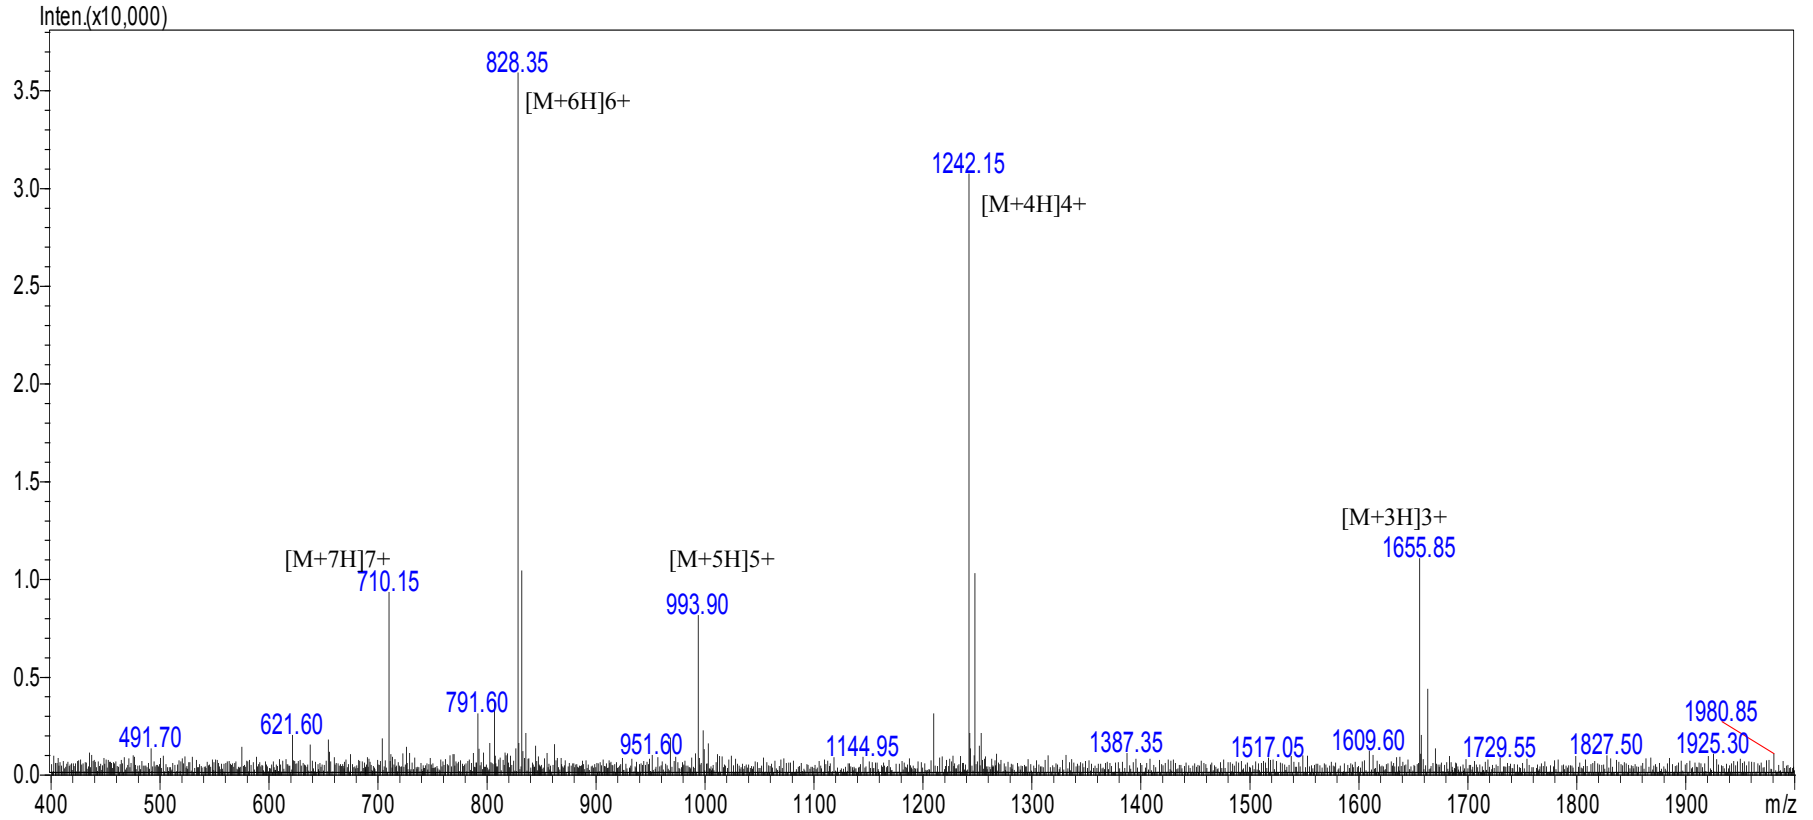

Date and Time: 2019-11-25 9:04:23  
Sample : TB500  
MW : 4963.55  
Lot No. : P191120-YS055820

Probe: ESI  
Nebulizer Gas Flow: 1.5L/min  
CDL: -20.0v  
CDL Temp: 250°C  
Block Temp: 200°C

Probe bias: +4.5kv  
Detector: 1.5kv  
T. Flow: 0.2ml/min  
B. conc: 50%H2O/50%ACN