


HPLC TEST RESULT

DSIP

Product Name: DSIP
 Lot No: P210622-LR055319
 Column: Xbridge BEH130 C18, 4.6*250mm, 5um
 Solvent A: 0.1%Trifluoroacetic in 100% Acetonitrile
 Solvent B: 0.1%Trifluoroacetic in 100% Water
 Gradient:

	A	B
0.0min	9%	91%
25.0min	34%	66%
25.1min	100%	0%
30.0min	stop	

Flow Rate: 1.0ml/min
 Wavelength(nm): 220nm

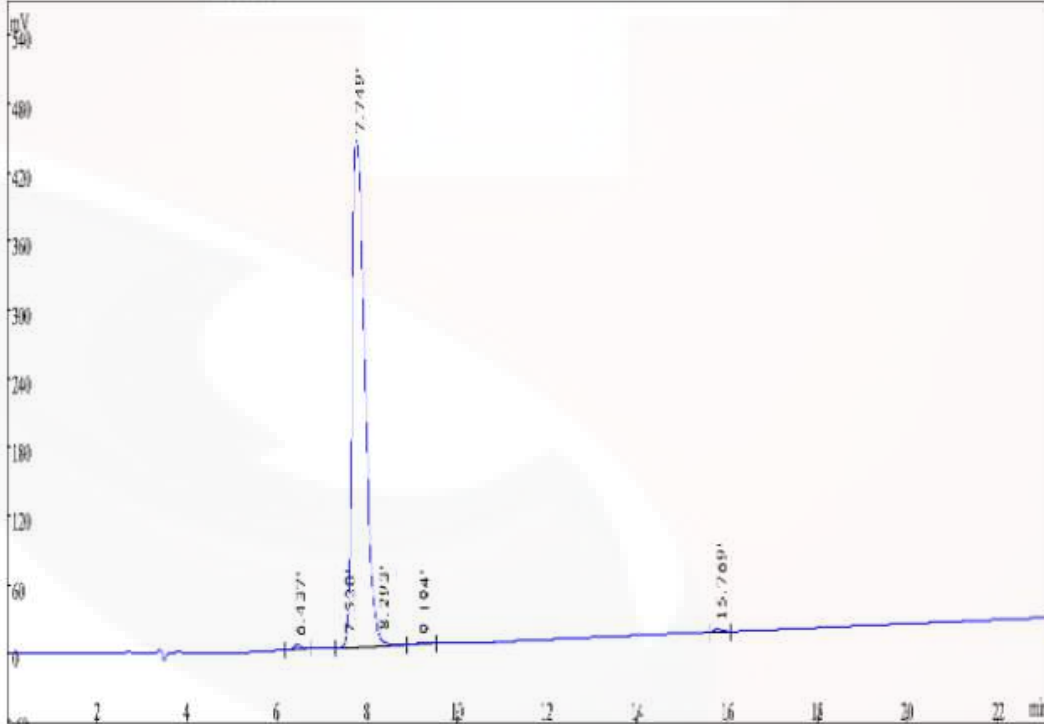

Rank	Time	Quantity	Area	Height
1	6.437	0.4676	38929	3770
2	7.520	0.1286	10705	5531
3	7.749	98.21	8176484	442495
4	8.293	0.5727	47674	6141
5	9.194	0.2616	21777	1284
6	15.769	0.3576	29775	2701