


HPLC TEST RESULT

GHRP-6

Structure: GHRP-6
 Cas No : 87616-84-0
 Sequence: His-D-Trp-Ala-Trp-D-Phe-Lys-NH2
 Lot No: P191110-LR055254
 Column: Xbridge BEH130 C18, 4.6*250mm, 5um
 Solvent A: 0.1%Trifluoroacetic in 100% Acetonitrile
 Solvent B: 0.1%Trifluoroacetic in 100% Water
 Gradient:

	A	B
0.0min	26%	74%
25.0min	51%	49%
25.1min	100%	0%
30.0min	stop	

Flow Rate: 1.0ml/min
 Wavelength(nm): 220nm

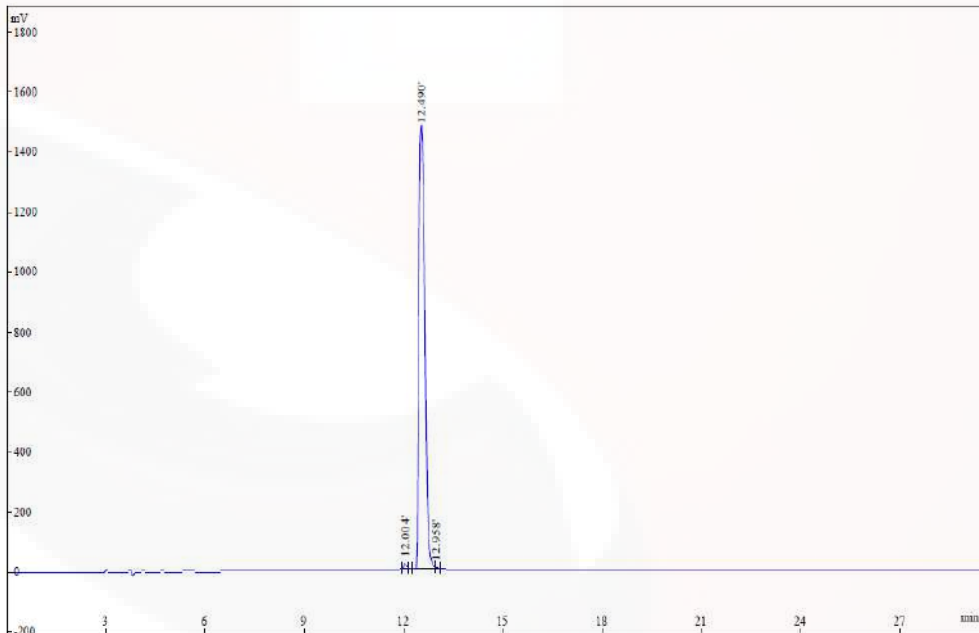

Rank	Time	Quantity	Area	Height
1	12.004	0.5482	101161	16545
2	12.490	99.3231	18329944	1483179
3	12.958	0.1287	23760	5712
Total		100	18454865	1505436