


HPLC TEST RESULT

MGF

Structure: MGF
Cas No :
Sequence: H-Tyr-Gln-Pro-Pro-Ser-Thr-Asn-Lys-Asn-Thr-Lys-Ser-Gln-Arg-Arg-Lys-Gly-Ser-Thr-P he-Glu-Glu-Arg-Lys-OH
Lot No: P191111-YS066649
Number: 0200049
Column: 250*4.6mm, Kromasil-C18-5um
Solvent A: 0.1%TFA in 100%water
Solvent B: 0.1%TFA in 100%acetonitrile
Gradient:

	A	B
0.1min	90%	10%
25.0min	65%	35%
25.1min	0%	100%
30.0min	stop	

Flow Rate: 1.0ml/min
Wavelength(nm): 220
Volume: 10ul

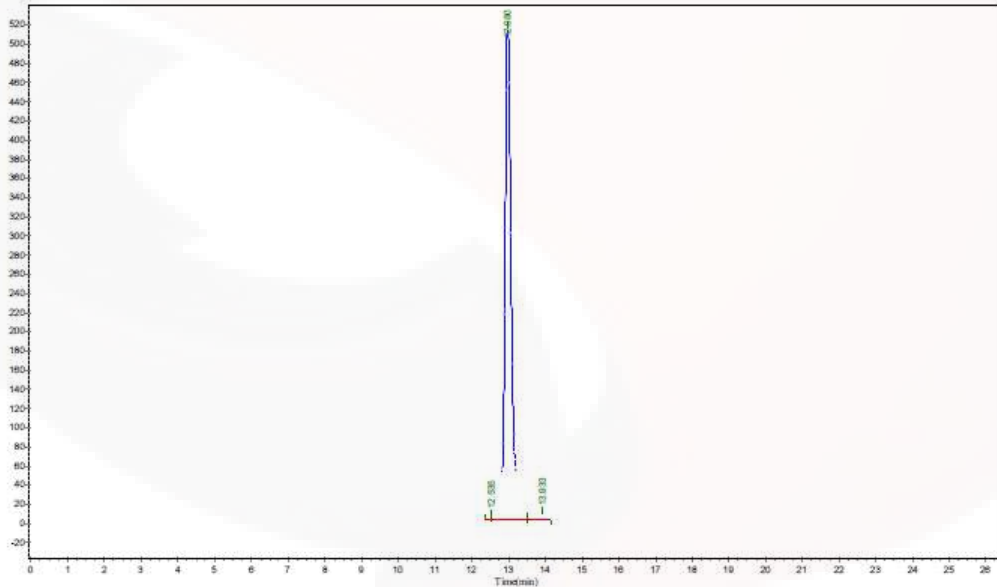

Peak No	Ret Time	Height	Area	Conc.
1	12.535	2805.786	10826.752	0.1738
2	12.980	512169.500	6163180.000	98.9425
3	13.933	4571.292	55047.469	0.8837
				100.00