


# HPLC TEST RESULT

## PEG-MGF

Structure: PEG-MGF  
 Cas No :  
 Sequence: PEG-Suc-YQPPSTNKNTKSQ(d)R(d)RKGSTFEEHK-NH2  
 Lot No: P191012-SY074059  
 Column: 4.6\*250mm, Boston Crest ODS  
 Solvent A: 0.1% trifluoroacetic in 100% acetonitrile  
 Solvent B: 0.1% trifluoroacetic in 100% water  
 Gradient:
 

	A	B
0.1min	15%	85%
25.0min	40%	60%
25.1min	100%	0%
30.0min	stop	

  
 Flow Rate: 1.0ml/min  
 Wavelength(nm): 220nm  
 Volume: 10µl

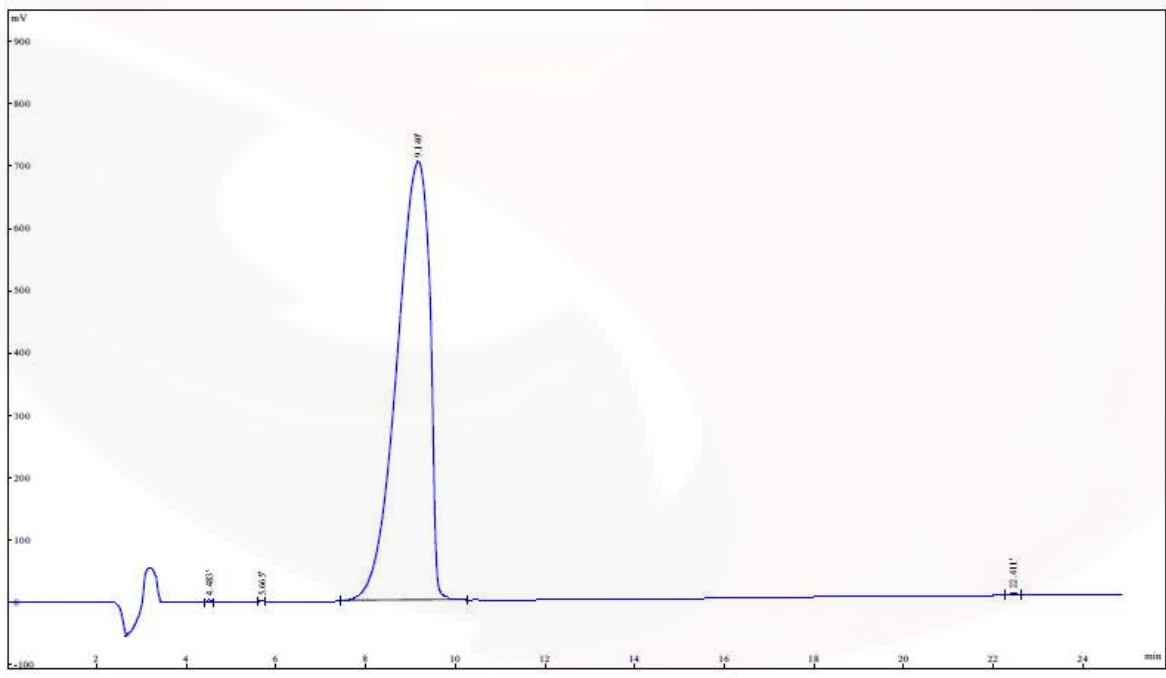

Rank	Time	Conc	Area
1	4.483	0.08265	29549
2	5.665	0.0429	15337
3	9.140	99.76	35666080
4	22.411	0.1153	41240
Total		100	35752206