

HPLC TEST RESULT

TB-500

Test Method:


Date: 4/10/21

Column : C18 4. 6*250mm, 5um
 Solvent B : 100% Acetonitrile
 Solvent A : 0.1% Trifluoroacetic in 100% Water
 Gradient :

	B	A
0.0min	10%	90%
30.0min	40%	60%

Flow Rate : 1.0ml/min
 Wave Length : 220nm
 Temperature : 37°C
 Concentration : 1.0mg/ml
 Sample Volume : 20ul

= Auto-Scaled Chromatogram:

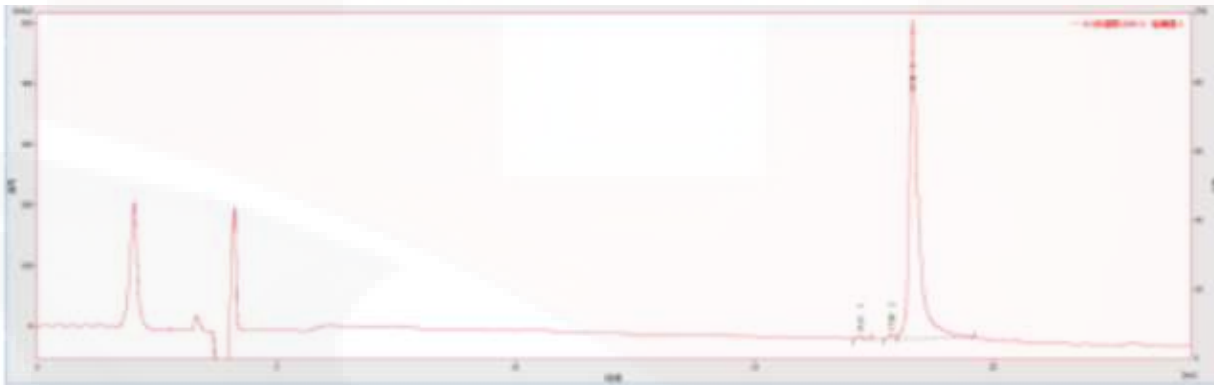

= Result:

	RT [min]	ST [min]	ET [min]	Area [mAU.s]	Area [%]
1	17.209	17.055	17.442	44.129	0.6
2	17.858	17.684	17.971	66.497	0.9
3	18.302	17.971	19.591	6934.067	98.4
	合计			7044.692	100.0